

FIG. 1
PRIOR ART

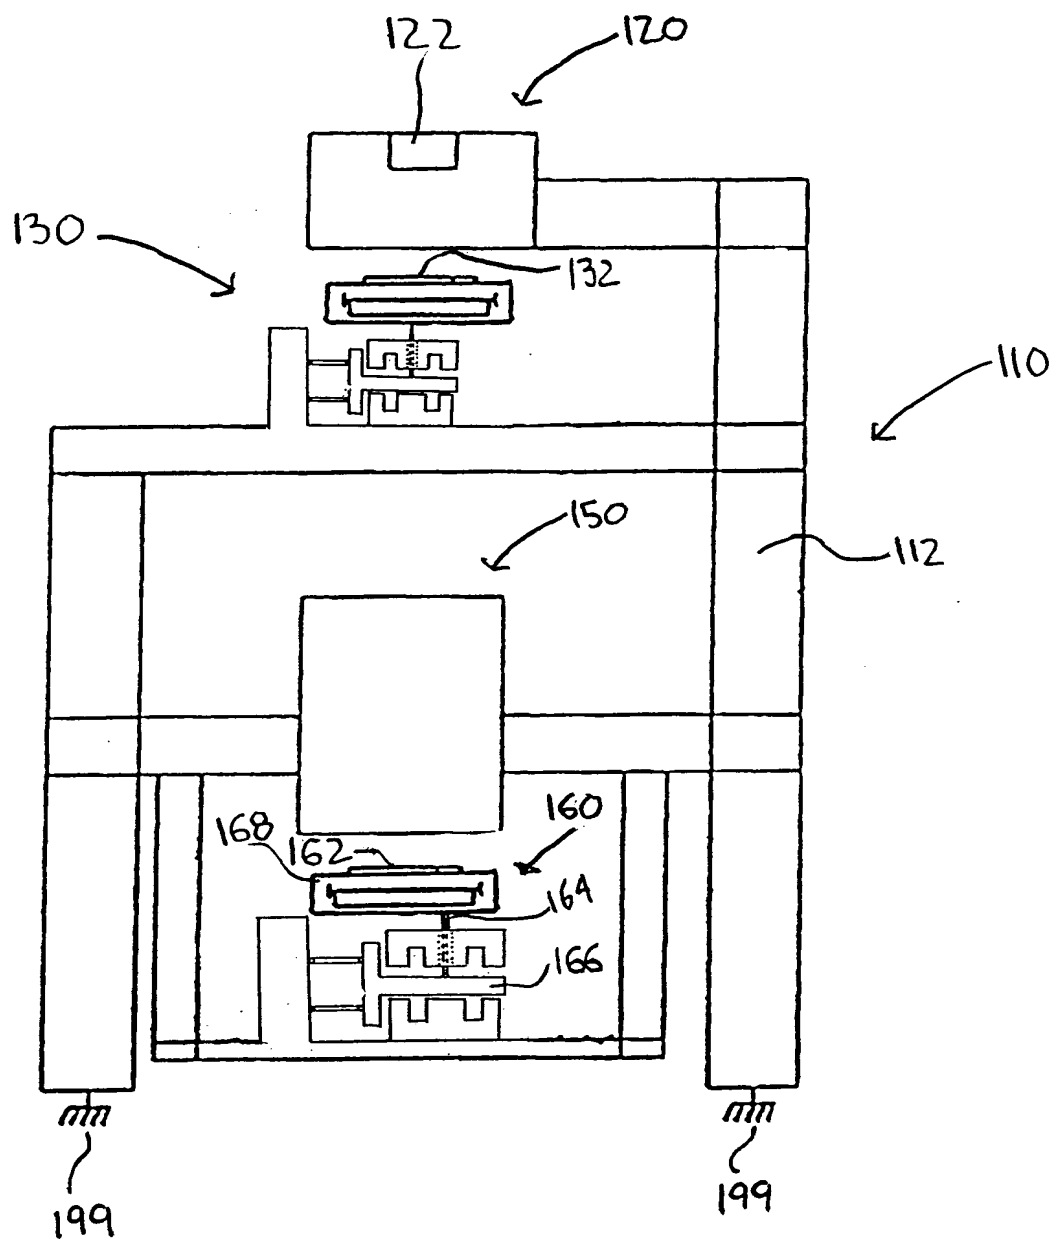


FIG. 2




FIG. 3 is a perspective view of the device 200.

202

204

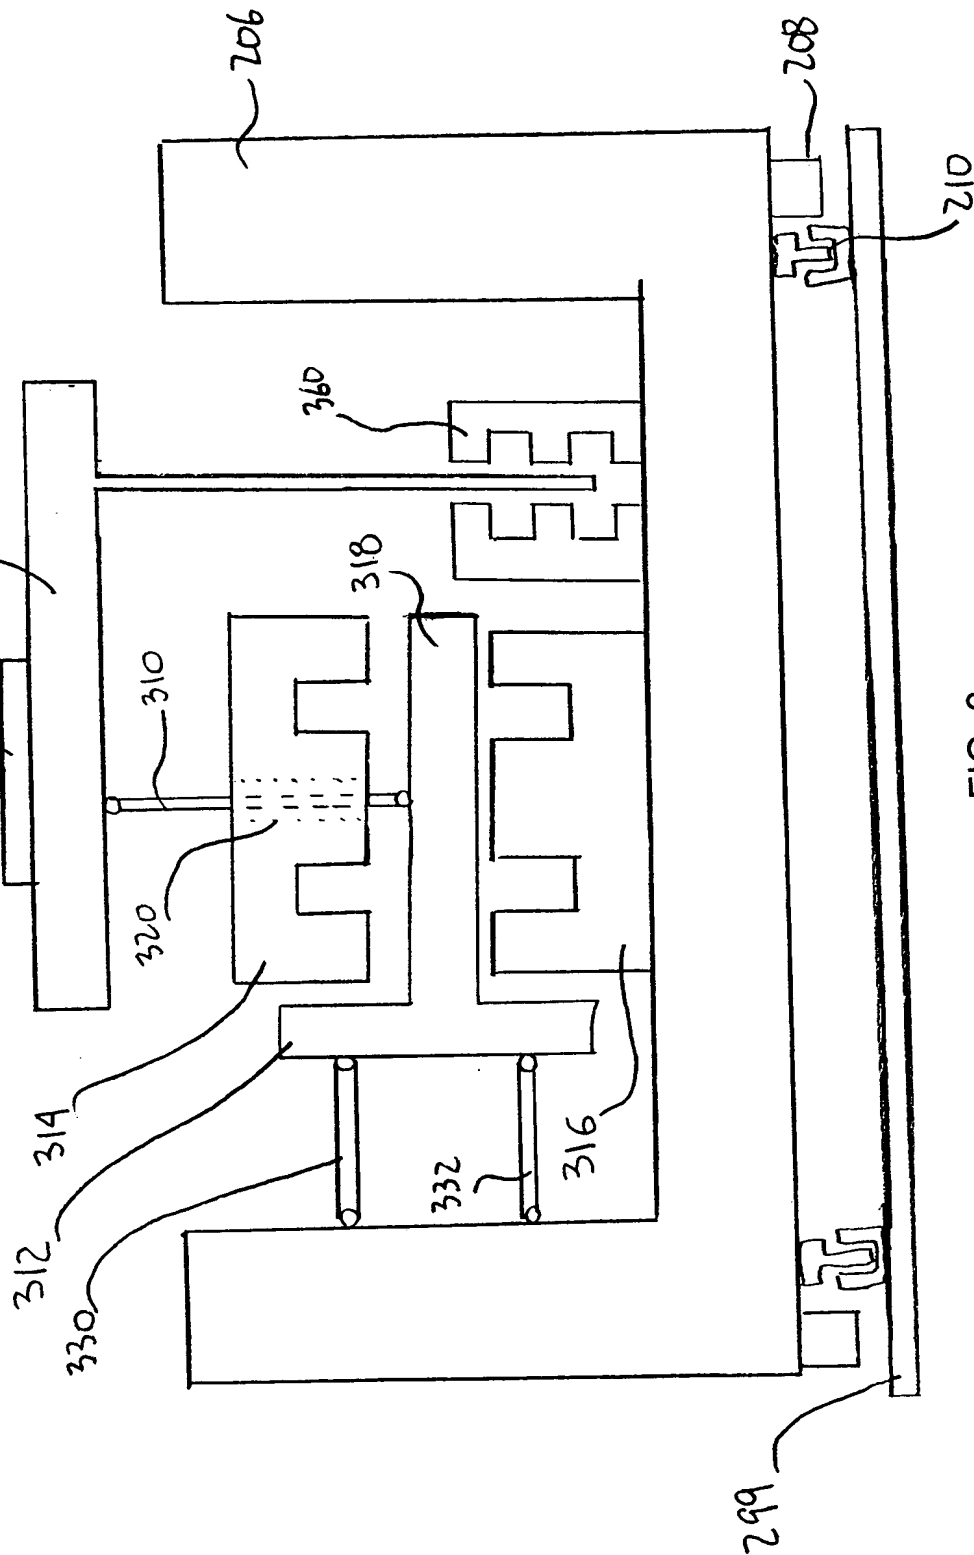


FIG. 3

FIG. 4 is a cross-sectional view of the device of FIG. 1, taken along the line 4-4 of FIG. 1, showing the device in a closed position.

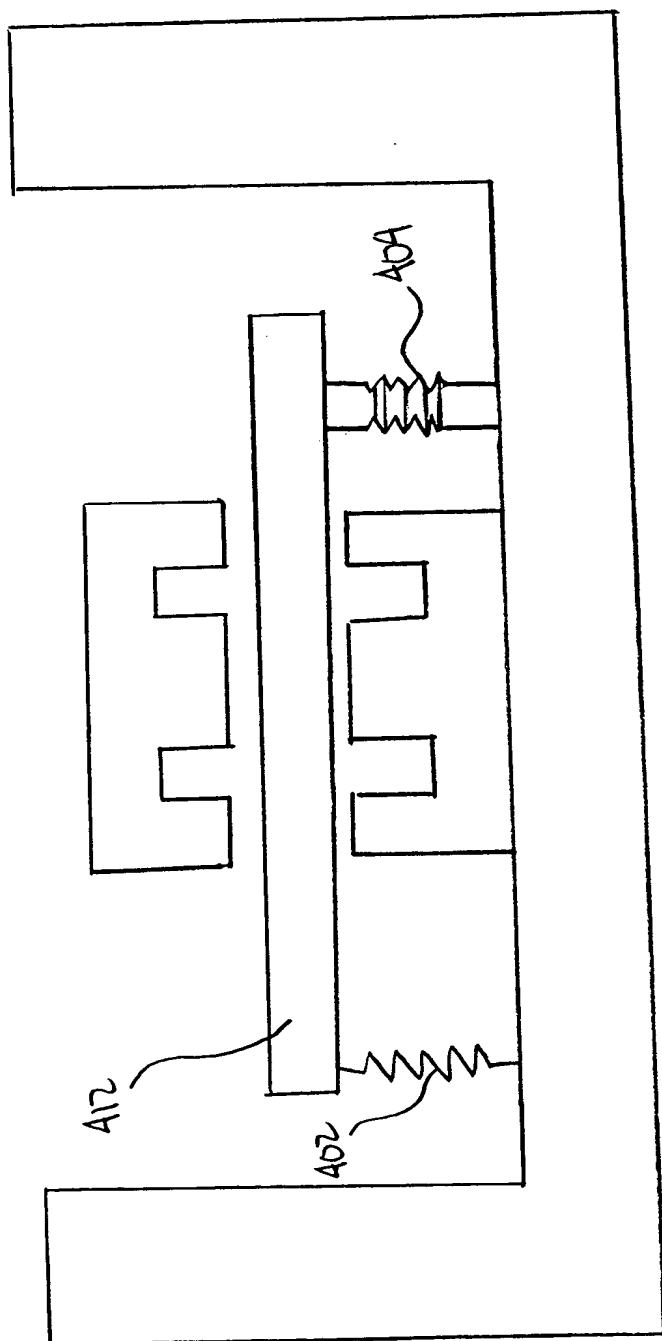


FIG. 4

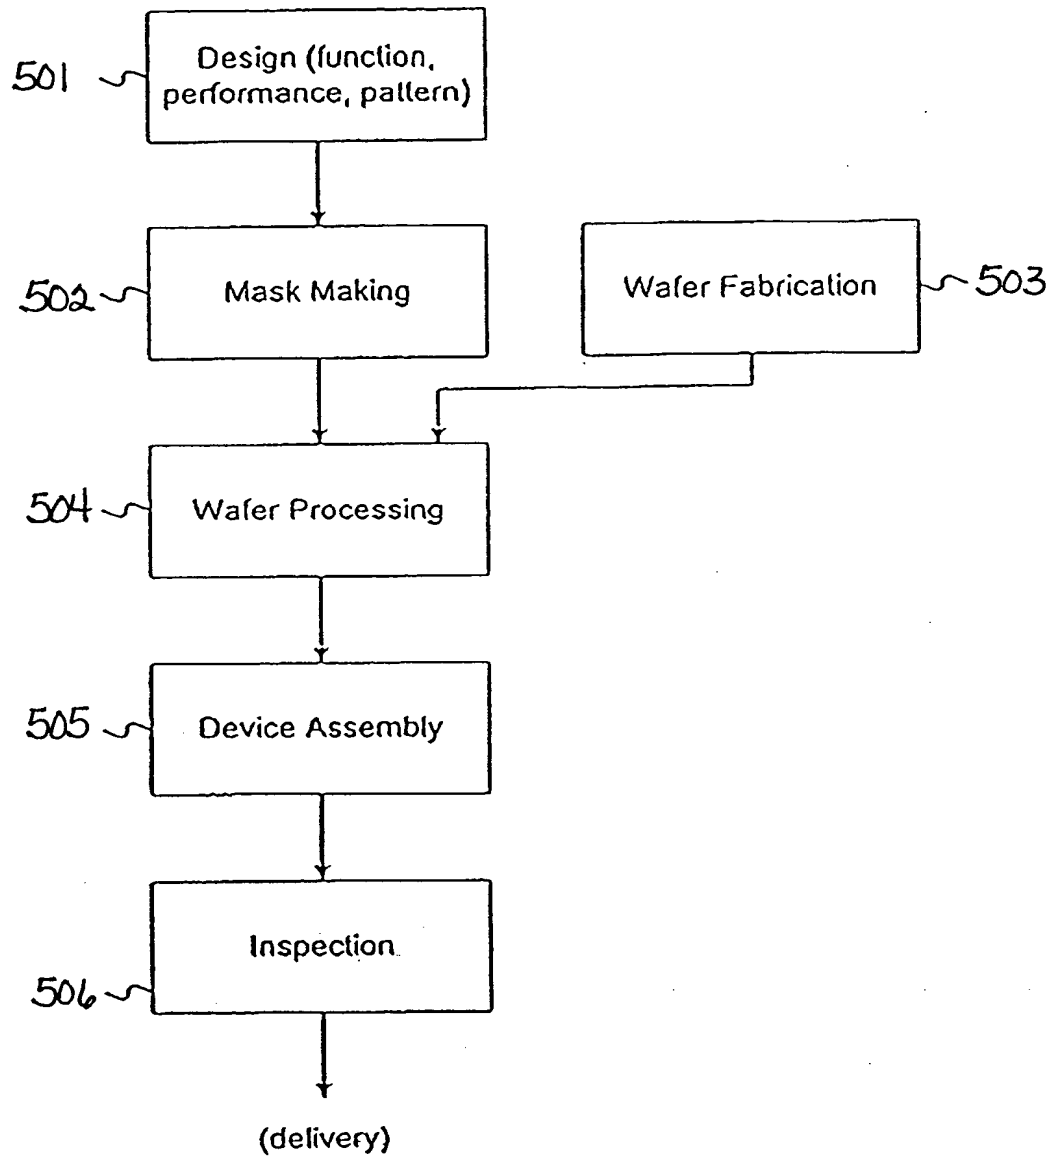


FIG. 5

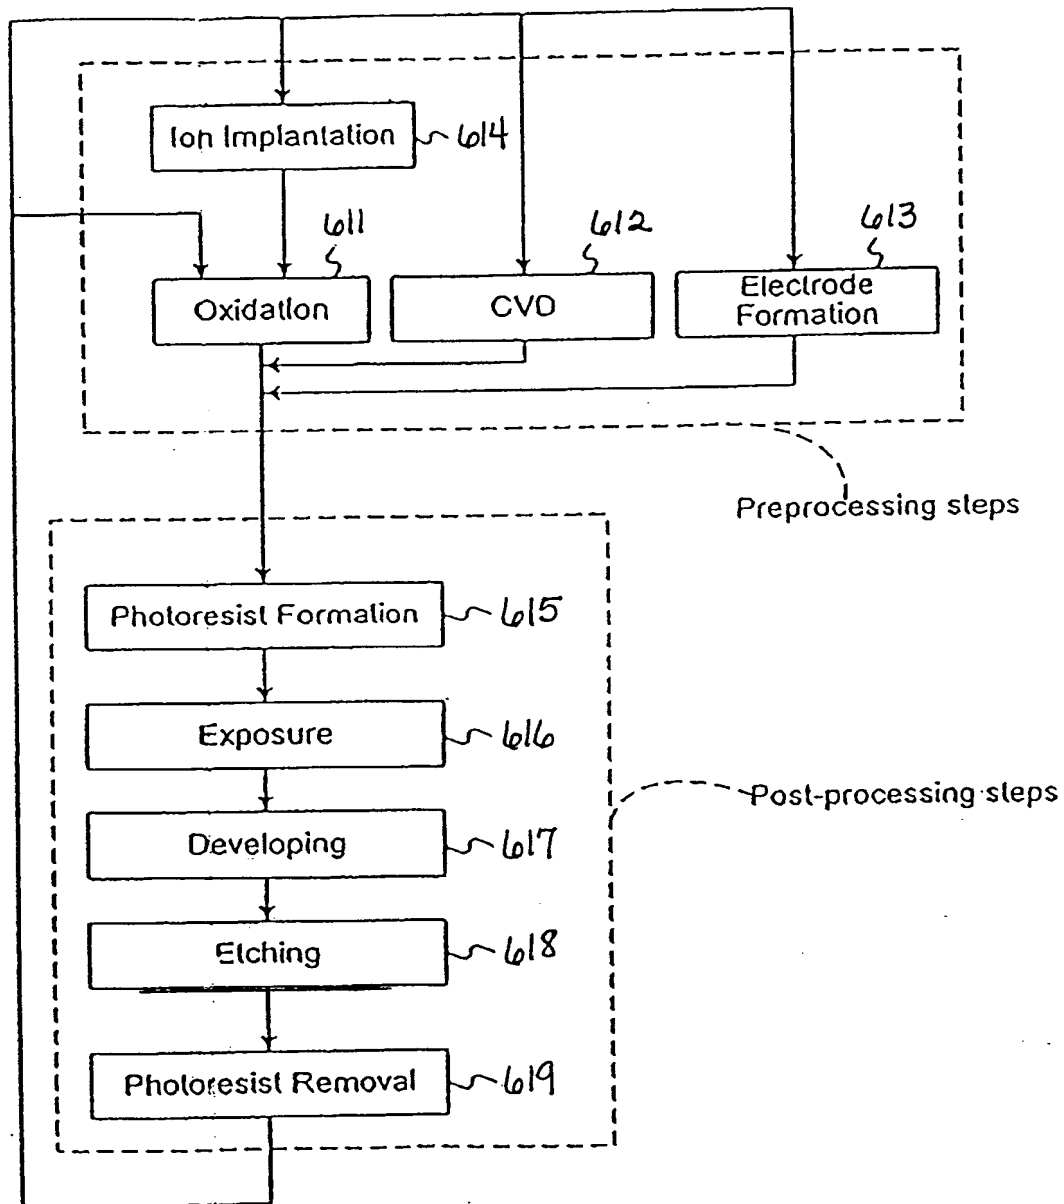


FIG. 6